


Analytical

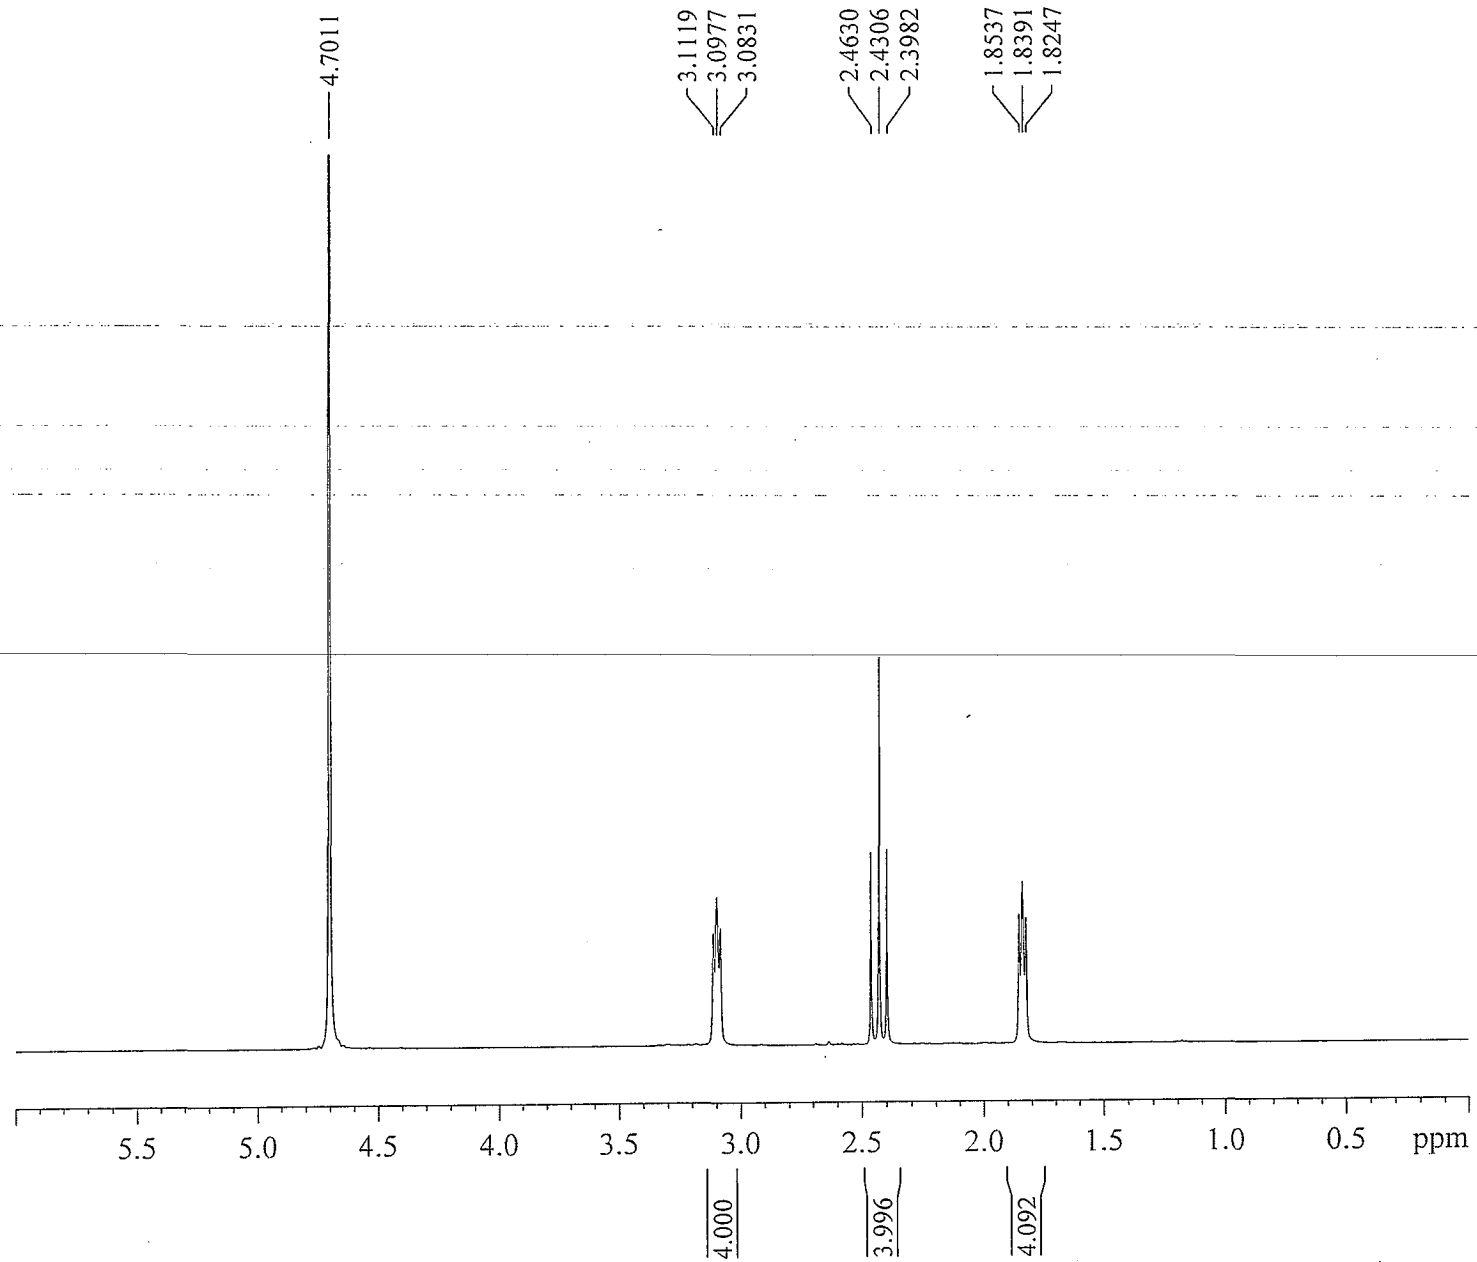

Current Data Parameters
NAME PBN2011404 PB177-110-01
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20140919
Time 10.28
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 65536
SOLVENT -D2O
NS 16
DS 2
SWH 8223.685 Hz
FIDRES 0.125483 Hz
AQ 3.9846387 sec
RG 128
DW 60.800 usec
DE 6.50 usec
TE 297.5 K
DI 1.00000000 sec
TD0 1

==== CHANNEL f1 =====
NUC1 1H
PI 12.66 usec
PLW1 20.00000000 W
SFO1 400.1324710 MHz

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

MS Spectrum

F:\MSDT SPC, time=2.753 of D:\CHEM32\1\DATA\2014-09\013(NEG) 2014-09-19 08:46:51\1A1-1701.D MM-ES+APCI, Pos, Scan, Fra

162.2

87.1

163.2

Max: 2.37056e+006